

QMC Instruments Ltd

Cryogenic Detector System



Operating Manual

Model QGeGa/2

CONTENTS

First – A Word of Warning

Introduction

- The System. Type QGeGa/2
- The Type QGeGa/X Photodetector
- The Filters
- The Preamplifier
- Serial Numbers

Packing List

1. Unpacking and Preparing the System for Operation

- Initial Inspection
- Removing the transit-plate
- Cryostat visual inspection
- Fitting the cryostat base-plates

2. Evacuating the Cryostat

3. Liquid Nitrogen Pre-cool

- A note about vacuum pumps
- The need to pre-cool with liquid nitrogen
- Safety valves
- The liquid nitrogen pre-cool period
- Removing the liquid nitrogen from the central reservoir

4. Liquid Helium Transfer

- The liquid helium transfer tube
- Helium gas recovery
- Keeping the cryostat cold
- Notes on running the detector system

5. The ULN95 Preamplifiers

- Preparing the preamplifiers
- Powering the preamplifiers
 - Power option a) Using an external power supply
 - Power option b) Using the internal batteries
- Recharging the batteries
- Adjusting the detector bias conditions
- Troubleshooting

6. System Calibration and Test Results

- System Cryogenic Performance
- Detector Test Results

Appendix A. The Gallium Doped Germanium Photoconductor

Appendix B. System Test Log Sheet

Appendix C. Filter Transmission

Contract Details and Guarantee

First - A Word of Warning

Lifting and Handling the Cryostat

Please take care when moving and lifting the system. The cryostat is designed to offer the best possible environment for your detectors and at the same give good cryogenic performance for your convenience. It is, as a consequence, rather heavy.

Using Cryogens

Cryogenic liquids are potentially dangerous. If you are not already familiar with the standard procedures appropriate for the use of liquid nitrogen and liquid helium, please seek advice before proceeding.

Operating this equipment involves the use of vacuum and cryogenic liquids. Please read this manual carefully before you operate the system – although this is not a safety instruction manual, the text describes our own procedures and this may help to avoid accidents.

The photo below shows part of a system that was pressurised because the boiling helium could not escape. We do not want this to happen to you. Please ensure that all personnel involved in the use of the detector system are fully accustomed with the techniques involved.



Introduction

- **The System. Type QGeGa/2**

This is a QMC Instruments Ltd. detector system type QGeGa/2 which incorporates a fast Gallium doped Germanium photoconductor. The detector is mounted in an optical integrating cavity behind Winston Cone optics and is restricted in bandwidth using appropriate multi-mesh low-pass filters. These components are mounted in a type TK1813 liquid helium cryostat built to our specification by our sister company Thomas Keating Ltd.

- **The Type QGeGa/X Photodetector**

This detector is an extrinsic germanium photoconductor designed for operation at 4.2K. The germanium chip is doped with gallium by exposure to a high energy neutron source. When biased this offers high sensitivity and speed of detection in the region bounded at low frequency by the photoconductivity edge at approximately $120\mu\text{m}$ (83cm^{-1}) and at the high frequency by the low-pass filters mounted in this system, in this case at about $23\mu\text{m}$ (430cm^{-1}).

- **The Filters**

Unrivalled cryogenic efficiency and broad-band transmission efficiency is achieved using our unique multi-mesh filter technology (product code QMMF) which is used on both the liquid nitrogen radiation shield (77K) of the cryostat and on the entrance aperture of the Winston Cone (at 4.2K). The filter mounted at 77K greatly reduces the radiative heat load on the liquid helium cooled stage of the cryostat from room temperature objects. It achieves this by cutting off sharply at the upper limit of the observing band and then reflecting the vast majority of higher frequency power. The measured transmission spectra of this particular filter is presented in **Appendix C**.

- **The Preamplifier**

The system incorporates a ULN95 preamplifier. This is mounted on the side of the body of the cryostat to reduce signal interference. The preamplifier can be powered either by internal rechargeable NiCd batteries or by an external power supply. The circuit includes a bias potentiometer and a number of test / monitoring facilities for ease of operation.

- **Serial numbers**

Item	Serial Number
QGeGa/2 detector system	XXXX
QGeGa/X detector	XXXX
ULN95 preamplifier	XXXX
TK1813 cryostat	XXXXX-X

Packing List

The following items are included in this shipment. Please check the contents against this list and contact QMC Instruments as soon as possible if you suspect that any items are damaged or missing.

Detector System Type QGeGa/2

- Type TK1813 cryostat containing:
 - Detector type QGeGa/X
 - Cold condensing optics. f/3.5 Winston Cone with 15mm diameter entrance aperture
 - SMA electrical connection into the cryostat
 - Low-pass type QMMF filters mounted on the Winston Cone at 4.2K and on the 77K shield aperture
- Cryostat fitted with:
 - Transit protection fixtures
 - Over-pressure relief valve fitted to the cryostat top plate for safety
 - Non-return valve
 - Two-off preamplifier mounting screws
- Cryostat central neck safety baffle which includes:
 - Over-pressure relief valve
- ULN95 preamplifier with:
 - Power supply lead
 - Rechargeable NiCd battery pack
- Outer vacuum case base plate with O-ring
- 77K radiation shield base plate
- Liquid nitrogen blow-out tube
- Spares kit which includes:
 - O-rings
 - Set of screws
 - ULN95 preamplifier power supply lead and spare 500mA fuses
 - M3 and M4 Allen keys
- Operating manual

1. Unpacking and Preparing the System for Operation

The system is not supplied in a condition that renders it ready for immediate use. A temporary base-plate has been installed to protect the system from damage during its journey. The following procedure must be carried out to prepare the detector system for operation. To prepare the system for transportation the following procedure should be followed in reverse.

Photographs included in this manual are general photos that may not be specific to your particular system.

Initial Inspection

Please inspect the box in which the goods were shipped, and the contents, for any obvious sign that damage has occurred in transit. If you think that the package has been damaged in some way, please contact us before proceeding further. Your equipment is guaranteed for two years against failure resulting from effects beyond your control, and we will be happy to make any repairs at no cost to you during this time.

The O-rings, bolts, screws etc, that are required to prepare the system, can be found in the spares kit.

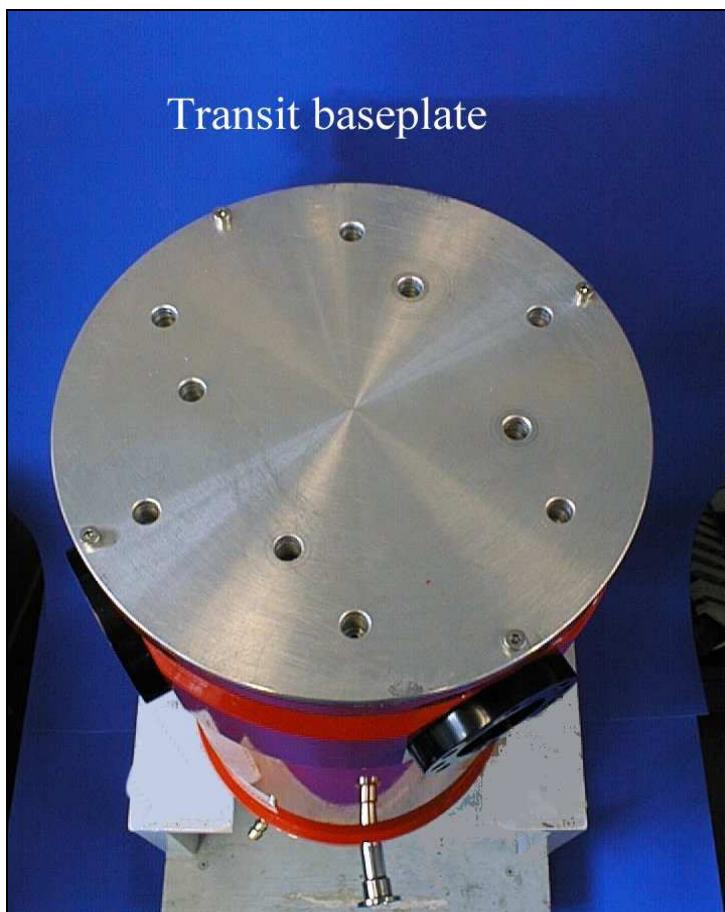


Photo 1.1. Transit base-plate

Removing the Transit Plate

Refer to Photo 1.1

To allow access to the bottom-plate, invert the cryostat so that it rests on the stainless lifting ring. To avoid marking the ring, stand the system on something to protect it such as soft tissue, cloth or bubble wrap.

The aluminium transit base-plate should be removed by unscrewing all the socket head screws holding it in place and carefully lifting it from the cryostat.

Cryostat visual inspection

Refer to Photo 1.2

Taking care not to disturb the wires that run along the work surface, remove the four support pillars.

The detector block is bolted onto the cold-plate with the Winston Cone attached to it. There are two filters, one of which can be found mounted onto the end of the Winston Cone and held in place by a press-fit filter cap which is also located with low temperature varnish; the other filter is located in the optical aperture of the liquid nitrogen shield. It is important for good detector performance that the detector / cone assembly is in good thermal contact with the work surface. You should confirm that the detector block is firmly screwed in position and that the filters have not worked loose in transit. It is possible that vacuum grease that is used to ensure good thermal contact of the detector block with the cold-plate, and small flakes of hardened GE varnish, which is a yellow substance used to glue the wires to the cold-plate, may be found in the cryostat. This is quite normal and will not give rise to operating difficulties.



Photo 1.2. The four support pillars and the detector optics

Fitting the cryostat base-plates

Refer to Photo 1.3 and 1.4

The TK1813 cryostat has a liquid nitrogen cooled 77K radiation shield base-plate, and a room temperature outer vacuum casing (OVC) base-plate. The 77K shield is located using the set of M3 screws provided. The black OVC base-plate is located using the M4 socket headed screws provided. It is important to check that the O-ring is in place, that it is clean, well greased and that its seating is free of marks and scratches. The screws locating the OVC base-plate should not be over-tightened because this can distort the O-ring and may cause vacuum leaks. If the screws are equally tightened, it is normal for a small gap to show between the lip of the OVC base-plate and the bottom of the cryostat casing.

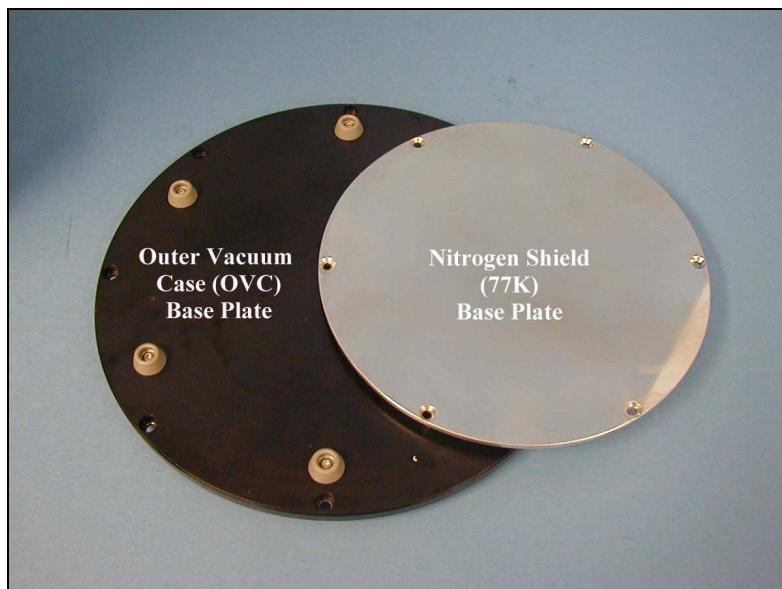


Photo 1.3. Cryostat base-plates



Photo 1.4. Liquid nitrogen base-plate in position

2. Evacuating the Cryostat

Please refer to **Photo 2.1.** Before cooling the cryostat, the vacuum chamber must be evacuated by connecting a suitable pump to the evacuation port located on the top-plate. The pump should be capable of reducing the pressure in the cryostat to below 10^{-1} mbar. This can with time be achieved by using a rotary pump only, but for optimum cryogenic performance of the cryostat it is better to use a diffusion or turbo-molecular pump to reduce the pressure still further.

The pumping system should ideally have a pressure gauge measuring the pressure as close to the cryostat as possible. The spare NW16/KF16 port located on the top-plate of the cryostat can be used to attach a pressure gauge to monitor the pressure in the cryostat directly.

Always check the quality of the pump system and pumping line prior to opening the cryostat valve.

The vacuum valve should be opened very slowly when the pressure in the cryostat is at or close to atmospheric pressure. This prevents rapid pressure changes that risk damage to the delicate components inside the cryostat.

Typically, the system could be ready for pre-cooling (refer to Section 3) after pumping for thirty minutes using a two stage pumping station.

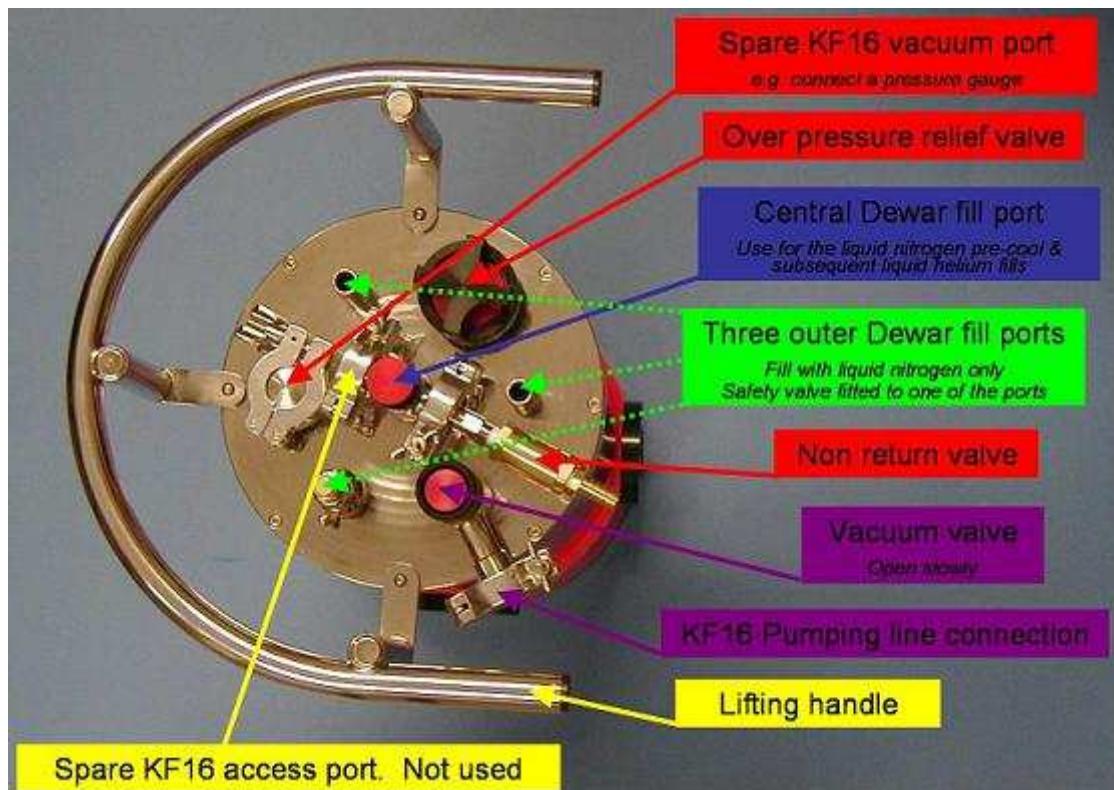


Photo 2.1. Cryostat top-plate fittings

3. Liquid Nitrogen Pre-cool

IMPORTANT: Refer to the warning at the front of the manual before proceeding with cryogenic cooling of this system.

A word about your vacuum pump

The pressure in the cryostat should drop rapidly when filling with liquid nitrogen because some of the gas, mainly oxygen, begins to cryopump (condense onto the cold surfaces). The system can remain attached to the pump during the pre-cool period if the pump you are using is an oil diffusion or turbomolecular type pump with a base pressure lower than 10^{-6} mbar. If you are only using a rotary pump, then the pressure in the cryostat will be lower during the pre-cool period than the pump is capable of generating, and the pump must therefore be detached immediately prior to cooling.

The need to pre-cool the central reservoir with liquid nitrogen

When a satisfactory pressure has been reached in the cryostat vacuum chamber, it is necessary to pre-cool the cryostat with liquid nitrogen before cooling with liquid helium. This will reduce the amount of liquid helium used.

Fill both the liquid nitrogen and liquid helium reservoirs with liquid nitrogen using the appropriate ports, **photo 2.1**. Liquid nitrogen need only be poured in through one of the three liquid nitrogen ports. The neck baffle assembly should be unscrewed and removed from the central liquid helium port to enable the liquid nitrogen cryogen to be poured into the liquid helium reservoir.

For preference, transfer the liquid nitrogen directly from a pressurized liquid nitrogen storage Dewar which should take around 15 minutes to complete. Alternatively, pour the liquid nitrogen using a bucket and a funnel, as shown in **photo 3.1**, which may take in excess of an hour to complete. In this case, the funnel must be attached to a pipe which extends down into the neck and well into the reservoir itself. For a TK1813 cryostat a length of at least 200mm is needed. The pipe diameter should be about 6mm (1/4 inch) to allow both reasonable throughput and space outside of the pipe for boiling nitrogen gas to escape.

Safety valves

The top-plate fittings are shown in **photo 2.1**. The helium reservoir access port should always be fitted with the non-return valve to stop the condensation of moisture within the neck. This moisture could freeze and block the neck of the cryostat which in turn could lead to failure and damage.

The cryostat neck baffle is shown in **photo 3.2**. The baffle incorporates an overpressure release valve. Should an ice blockage form in the central neck of the cryostat, gas will be unable to escape through the non-return valve. Such an event will cause the overpressure relief valve, located at the top of the baffle, to open thereby releasing pressure from the inner reservoir.

The pre-cool period

The length of pre-cool period will determine the initial efficiency of use of liquid helium. For a TK1813 we recommend a minimum pre-cool of four hours, but it is often convenient to leave a cryostat overnight if, for example, it has been attached to a pump throughout the day. Larger cryostats (TK1840, TK1865 and TK1875) require a longer minimum pre-cool period because the additional gas cooled radiation shield is only weakly linked to the other temperature stages and therefore cools slowly. For these larger cryostats, a twelve hour minimum pre-cool period is recommended.



Photo 3.1. Using a funnel to fill the cryostat with liquid nitrogen



Photo 3.2. Cryostat neck baffle

Removing the liquid nitrogen from the central reservoir

When the pre-cool period is complete the liquid nitrogen in the helium reservoir should be removed. This is best done using a supply of compressed dry nitrogen gas and the blow out tube supplied. The O-ring and tightening ring from the central reservoir access port, and brass washer from the spares kit, should be arranged on the blow out tube as shown in **photo 3.3**. The non-return valve should be replaced with the adaptor nozzle. The liquid nitrogen can now be removed from the central reservoir by applying (through the adaptor nozzle) a small overpressure within the reservoir as shown in **photo 3.4**. The liquid nitrogen is directed into a safe container, and can be used to replenish the outer reservoir.

It is important that all of the liquid nitrogen is removed from the central reservoir before the liquid helium transfer is started. Any liquid nitrogen remaining in the central reservoir will be frozen by the

liquid helium. Nitrogen ice forms an effective insulating layer which will prevent the detector reaching its intended operating temperature. A large amount of expensive liquid helium will also be wasted in creating a small amount of very cold nitrogen ice!

The supply of dry nitrogen gas can be continued until the stream of ejected liquid nitrogen ceases. Ensure that the blow out tube does not block, that it is properly located and it reaches the bottom of the helium reservoir. The Germanium thermistor resistance increases exponentially as the temperature falls reaching a resistance of approx tens of $k\Omega$ at 4.2K. Note that there is little change in impedance of the GeGa thermistor above 10K, and that the resistance of the coaxial wiring exceeds that of the Ge detector at higher temperature.

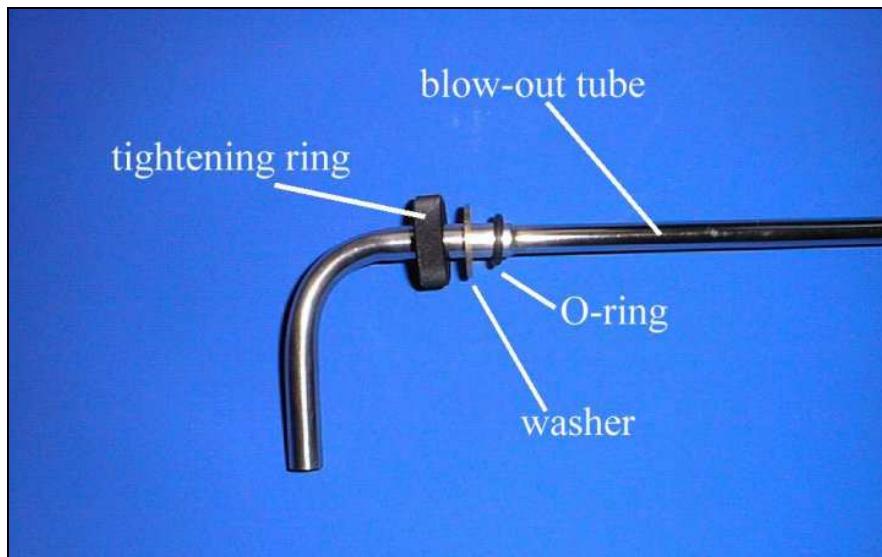


Photo 3.3. The blow out tube

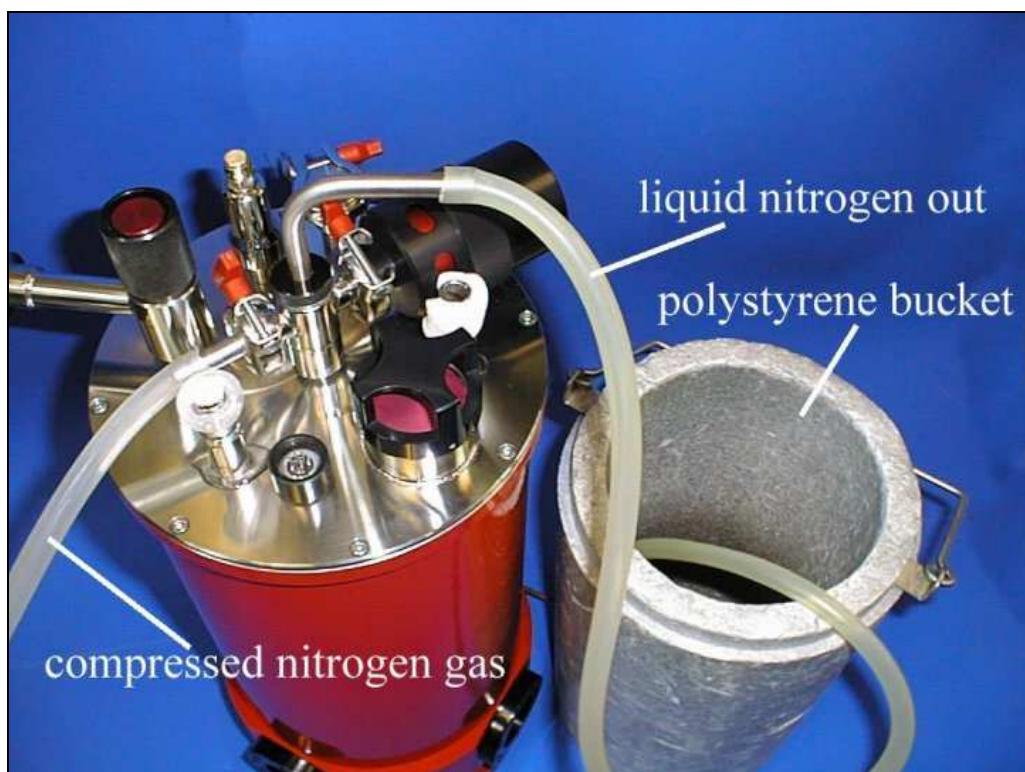


Photo 3.4. Arrangement to blow the liquid nitrogen out of the liquid helium reservoir

4. Liquid Helium Transfer

When you are certain that all liquid nitrogen has been removed from the central reservoir the cryostat can be filled with liquid helium. The blow-out tube should be removed from the central neck and the cryostat should be arranged such that the transfer tube reaches the bottom of the cryostat and the storage Dewar simultaneously.

It is wasteful to transfer liquid helium too quickly. A rubber bladder can be used to control the pressure driving the transfer, and the rate of filling can be judged from the size of the plume of exhaust helium gas rising from the cryostat.

The liquid helium transfer tube

It is important that the liquid helium transfer tube used is designed to suit both the detector cryostat and the liquid helium storage Dewar. The delivery end of the transfer tube should have a fully evacuated section with diameter approximately 6mm ($\frac{1}{4}$ inch) and length at least 200mm. It should therefore permit liquid helium to be delivered efficiently into the central reservoir while at the same time leave space for spent helium gas to escape without a build-up of pressure within the cryostat.

QMC Instruments Ltd. can arrange to supply a suitable liquid helium transfer tube for your cryostat. We offer a rigid transfer tube, product code QTT/R, and a flexible transfer tube, product code QTT/F, both with a horizontal reach in excess of 1000mm. Please contact us, or your supplier, if you have any questions regarding the suitability of your equipment.

Photo 4.1 depicts a liquid helium transfer in progress. **Photo 4.2** shows a typical boil-off plume in the phase when the cryostat is cooling between 77K and 4.2K. **Photo 4.3** shows the larger, cloudier and more erratic plume, which results when the liquid helium reservoir is full. At this stage the transfer should be terminated. It should take about thirty to forty minutes for a TK1813 cryostat to cool down from 77K to 4.2K and to fill with liquid helium; and the whole process should consume about four litres of liquid helium.

Helium gas recovery

Here in Cardiff we have no facilities for recovering spent helium gas, hence all the liquid helium transfers undertaken in our laboratories are “open” in the manner shown in the photos. However some installations offer recovery facilities whereby a helium return line is attached to the exhaust port of the cryostat. Use the black anodized aluminium tightening ring and O-ring from the central neck fitting to make a seal around the liquid helium transfer tube. Under such circumstances, a coarse flowmeter could be inserted in the return line to indicate flow rate from the transfer. Usually a steady flow-rate is indicated during the cool and fill phases of the transfer. When the reservoir is full however, the flow rate becomes erratic, and the transfer should be terminated.

When the transfer is complete the transfer tube should be removed carefully but swiftly and the safety valves fitted without delay. This kind of detector exhibits a rapid increase in resistance as it approaches liquid helium temperature and this can be used as a check on the final stages of the

transfer. The detector resistance can be measured by using a multimeter connected to the SMA input connector.



Photo 4.1. Liquid helium transfer



Photo 4.2. Helium gas exhaust during fill



Photo 4.3. Helium plume when complete

Keeping the cryostat cold

It is important to keep all the neck fittings and safety valves in place whenever the cryostat is cold. If these are removed for liquid helium transfer, they should be removed only at the last moment when all other preparations have been made. They should be replaced as soon as the transfer tube is removed.

The cryostat can be kept continuously cold by repeatedly replenishing the cryogens. Hold times for both the liquid helium in the central reservoir and liquid nitrogen in the outer reservoir are shown in **Table 6.1 in Section 6**.

Note that the liquid nitrogen in the outer reservoir will require topping up more often than the liquid helium, and that the first fill liquid helium hold time may be shorter. This is because the initial liquid helium boil-off rate may be high if significant further cooling takes place when the transfer is complete.

When transferring liquid helium into a cryostat that already contains liquid helium, the transfer tube should be fully cooled before it is inserted into the cryostat neck. This prevents the warm transfer tube and warm helium gas from boiling away excessive amounts of the liquid helium already in the cryostat. In this case the transfer tube is inserted into the storage Dewar and the pressure control bladder inflated slightly to pass gas through the tube to cool it. When the transfer tube has cooled, thick milky helium gas emerges from the delivery end, **photo 4.4**, and the transfer tube can then be manoeuvred carefully to the cryostat and lowered into the central neck. The refill can then proceed in the way described above.

Detector system operation

The detector system is ready for use as soon as the liquid helium fill is complete. The performance may improve very slightly during the first hour or so after the first fill liquid helium transfer while the detector and filters cool to their final operating temperature.

Remember that the resistance of the detector is a function of current once it is at operating temperature.



Photo 4.4. Liquid helium emerging from a cold tube

5. The ULN95 Preamplifier

Background

The ULN95 (Ultra Low Noise) preamplifier is a voltage mode low noise preamplifier designed for use with cooled detectors. It can be powered either from internal rechargeable batteries or from an external $\pm 15V$ DC supply. Switchable gain options, a potentiometer bias supply control and full detector status monitoring are provided. Output is 50Ω bnc as standard, and the circuit is housed in an RF shielded enclosure designed to mount directly to the detector cryostat to reduce interference and provide a common ground.

The input impedance is high, so the preamplifier can be used with a range of cooled detectors, including InSb hot electron bolometers (types QFI/X, QFI/XB and QFI/XBI), composite Silicon and Germanium bolometers (types QSIB/X and QGEB/X) and Gallium doped Germanium photoconductors (Type QGeGa/X).

The technical specification of the ULN95 is given in **Table 5.1** below.

Output impedance	50Ω bnc	Bias Supply:	0-10V multi-turn potentiometer
Input impedance	$>10G\Omega$	Voltage Gain:	x100, x1000 switchable
Bandwidth	0.5Hz to 1MHz	Output Noise:	$\approx 1nV Hz^{-1/2}$ rms $> 1kHz$ (input shorted) $\approx 3nV Hz^{-1/2}$ rms at 10Hz

Table 5.1. ULN95 Technical specification

Preparing the preamplifier

The preamplifier batteries have been disconnected for transit. Open the front of the ULN95 by unbolting the four bolts that hold the lid in place. The battery pack should be fixed in position as shown in **Photo 5.1a**, using the four nylon fixing screws.

The battery connecting lead, **Photo 5.1b**, which can only be fitted one way, should be connected to the 4-pin connector at the top of the left hand circuit board as viewed with the battery pack uppermost in the box. The preamplifier should be mounted onto the black anodised vacuum window surrounding the SMA electrical feedthrough which is located on the side of the cryostat. The two mounting bolts can be found screwed into this. Once mounted, the preamplifier SMA electrical input lead should be connected to the cryostat SMA electrical feedthrough through the hole in the lower section of the preamplifier housing, **Photo 5.1a**.

Powering the preamplifier

The ULN95 can be operated from the internal batteries or from an external power supply. External power is supplied via the 4-pin socket located at the top of the preamplifier control panel. The three isolated pins are used while the earth tag is not used. A twin channel power supply, an example of which is pictured in **Photo 5.2**, will be needed to run the preamplifier from external power. A power lead is supplied for this purpose. The internal NiCd batteries, which may not necessarily be charged before despatch, are recharged from the external power supply via the same socket. Please note that the NiCd rechargeable batteries will not be able to be recharged and used indefinitely. Through normal and proper use they will need replacing after about 200 charge/discharge cycles.

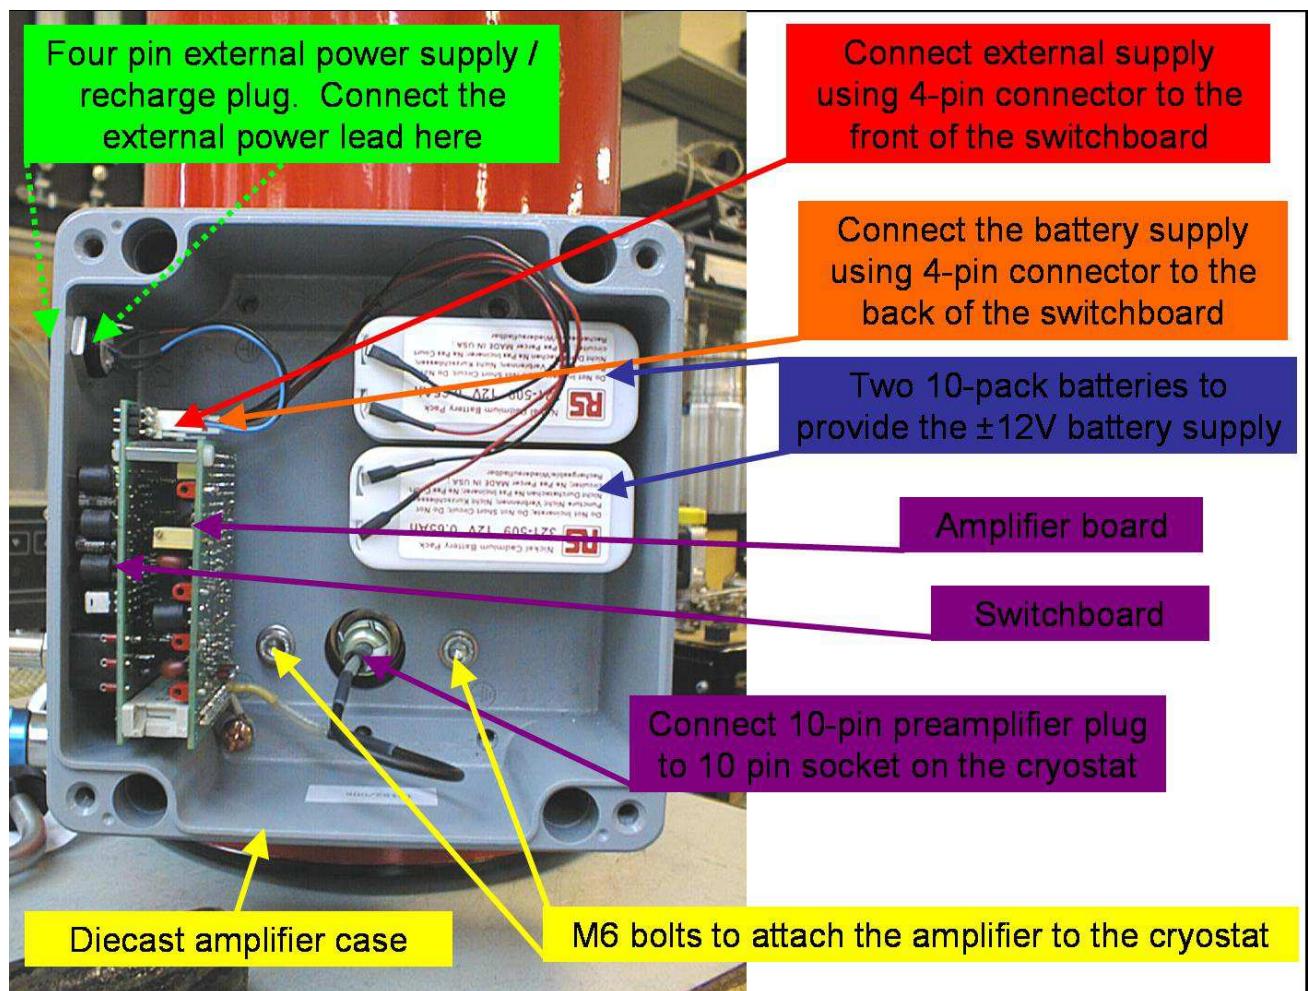


Photo 5.1a. Mounting the preamplifier to the cryostat

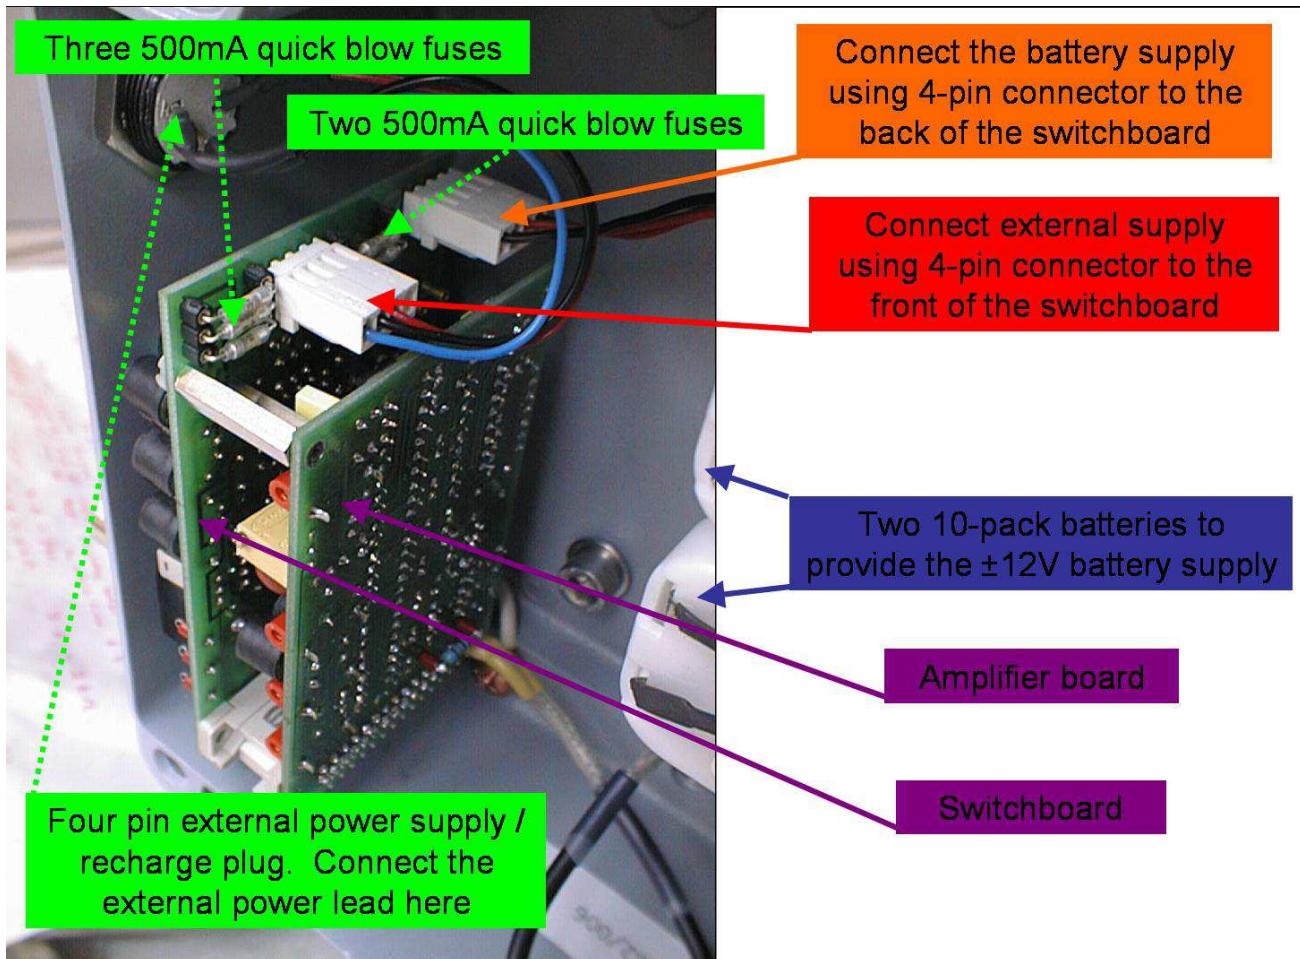


Photo 5.1b. Connecting the batteries

Power Option a) Using an external PS

Photo 5.2 shows a typical twin channel laboratory power supply which can supply 30V dc per channel. The photo also shows how the power lead supplied with the detector should be connected to such a supply.

When powering the preamplifier, make sure that the voltage output is at zero before switching on, and then increase the voltage gradually on both power supplies simultaneously to 15V.

If the power supply has a current limiting facility, this should be set to 200mA. The current supplied to the power socket is limited internally but occasionally transients can blow the 500mA protection fuses.

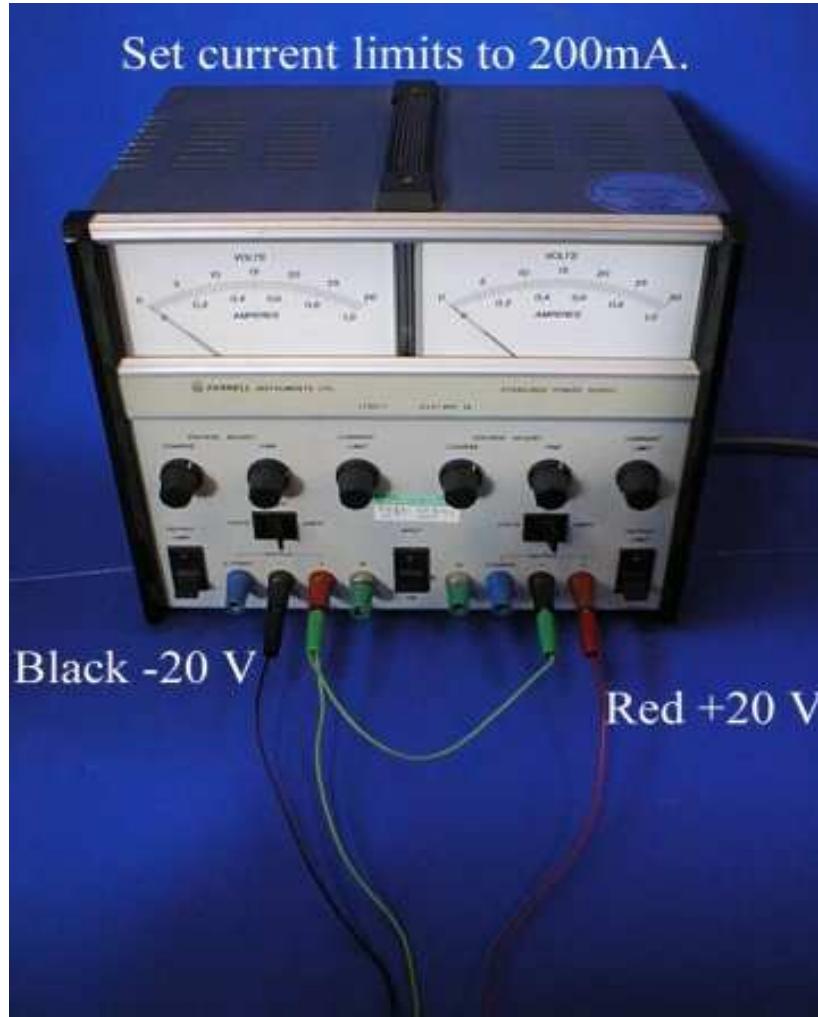


Photo 5.2. Power supply connections

External supply switch-on procedure is as follows from the following initial settings:

RECHARGE = OFF; POWER = EXT; INPUT = SHORTED; BIAS = OFF

1. Ensure that the power supply output voltages are set to 0V
2. Connect the power lead as shown in **Photo 5.2**. Plug the other end into the **RECHARGE SOCKET**
3. Increase the two output voltages to 15V gradually. The red **PREAMP ON** light should illuminate
4. Set the INPUT switch to the **OPEN** position
5. Set the BIAS switch to the **ON** position
6. Select the desired GAIN

At this stage, you can “Say Hello” to your detector. A hand waved rapidly in front of the detector window should generate a readily visible response on an oscilloscope.

Power Option b) Using the internal batteries

Battery supply switch-on procedure is as follows from the following initial settings:

RECHARGE = OFF; POWER = EXT; INPUT = SHORTED; BIAS = OFF

1. Set the POWER switch to **BATT**. The **PREAMP ON** light should illuminate
2. Set the INPUT switch to the **OPEN** position
3. Set the BIAS switch to the **ON** position
4. Select the desired GAIN

Fully charged batteries will be able to operate the preamplifier for at least 12 hours. However, this does depend to an extent on the level of output used. The power drain on the batteries is higher if the signal level is large.

Recharging the batteries

Battery recharge procedure is as follows from the following initial settings:

RECHARGE = OFF; POWER = EXT; INPUT = SHORTED; BIAS = OFF

1. Ensure that the power supply output voltages are set to zero
2. Connect the power lead as shown in **Photo 5.2**. Plug the other end into the **RECHARGE SOCKET**
3. Set the RECHARGE switch to **ON**
4. Increase the voltage to +/-15V as described above. The **PREAMP ON** light should illuminate
5. Increase the voltage gradually to +/-18V. The **RECHARGE ON** light illuminates brightly

Do not exceed a supply voltage of +/-20V. If you proceed according to these instructions it is not possible to overcharge the cells. The batteries will be fully charged when the recharge light goes out, which should take no more than eight hours.

You can operate the amplifier and recharge the batteries simultaneously.

When switching off, remember to switch the power option switch to external supply, otherwise the batteries will drain.

Altering the detector bias

Both detectors require a d.c. bias current I_B which is supplied by the preamplifier. I_B is set to the optimum value during testing at the QMC Instruments; hence it should not normally be necessary to alter the bias conditions of the detector. However, the bias conditions should be checked from time to time and adjusted if greater signal-to-noise can be achieved.



Photo 5.3. View of the switchboard and amplifier circuit board identifying the voltage test points and multi turn potentiometer

The bias voltage V_B supplied to the bias load resistor can be measured using the test points within the preamplifier box. On the board closest to the battery pack there are four test points and a variable resistor which are assigned, **photo 5.3**, as follows:

- TP1 Zero volt test point**
- TP2 V_B test point**
- TP3 I_B test point ($1\text{mV}/\mu\text{A}$)**
- TP4 Detector voltage test point, V_{Det}**
- VR1 V_B adjust**

To measure V_B connect a voltmeter across TP1 and TP2. To set V_B adjust the multi-turn potentiometer VR1. V_B will have been set at QMC Instruments Ltd during testing but can be altered using the potentiometer VR1 and measured between TP1 and TP2. To measure I_B connect a voltmeter across TP1 and TP3 and convert the measured voltage in mV to $I_B/\mu\text{A}$ using the conversion factor $1\text{mV}/\mu\text{A}$. V_{Det} is measured by connecting a voltmeter across TP1 and TP4. The operating resistance of the detector can then be calculated from $R_{\text{Op}} = V_{\text{Det}}/I_B$. Occasional monitoring of this voltage will confirm that the detector temperature and the bias current are correct and stable.

Figs. 5.1(a, b) give typical input shorted noise of the ULN95 amplifier at a gain of x100

Troubleshooting

If after recharging the battery packs performance starts to fall it is likely that the NiCd rechargeable battery packs will need replacing. It is normal for NiCd rechargeable batteries to need replacing periodically when they no longer hold charge. Replacement battery packs can be obtained from RS.

If problems are suspected with the ULN95 preamplifier there are some basic checks that can be carried out. Disconnect the ULN95 from the external supply and then open the box by undoing the four bolts. Check the following:

- Check the five 500mA fuses to make sure that they have not blown, **photo 5.4**
- The switchboard should be firmly attached to the RF shielded case
- The switchboard and amplifier board should be firmly attached to one another
- The SMA plug should be firmly attached to the cryostat SMA electrical feedthrough
- Confirm that the battery packs are firmly attached in position to the RF shielded casing, and that they are connected to the switchboard
- Confirm that there are no obvious problems with the switchboards and amplifier board. The boards can be detached and removed from the case for inspection. Check for any loose components or blackened areas

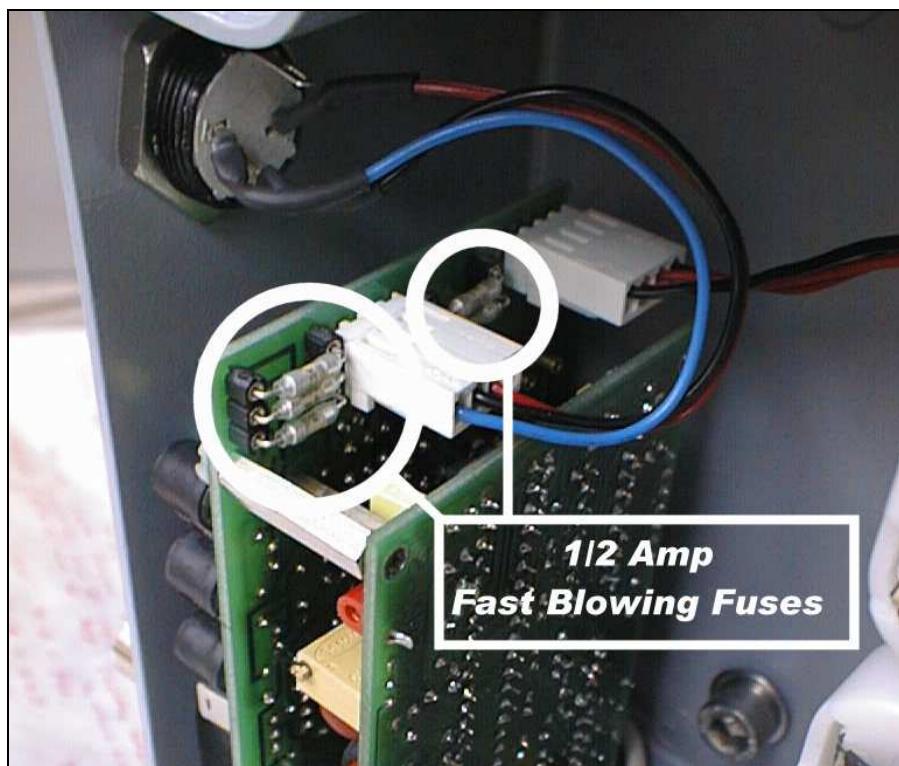


Photo 5.4. View of the switchboard and amplifier board, showing the location of the 500mA fuses

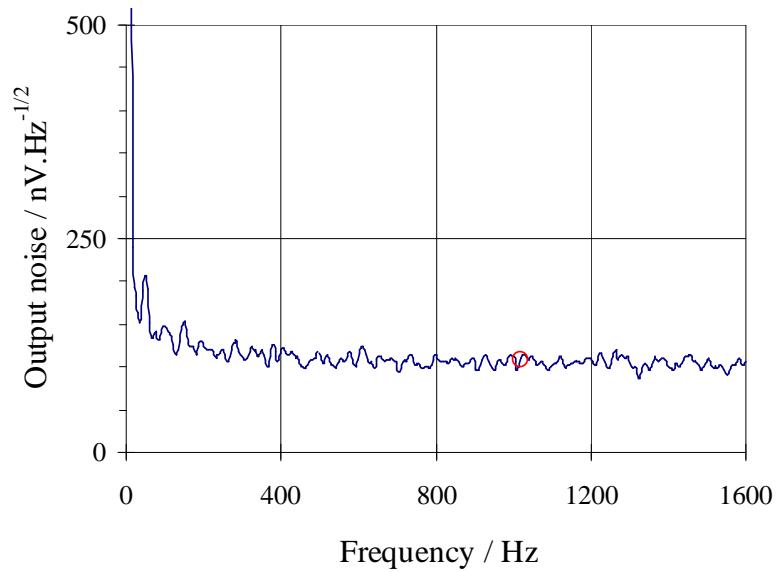


Fig. 5.1a. Typical preamplifier input shorted noise spectra at low frequencies
Amplifier gain = x100. Noise at 1kHz = 1.0nV.Hz^{-1/2}

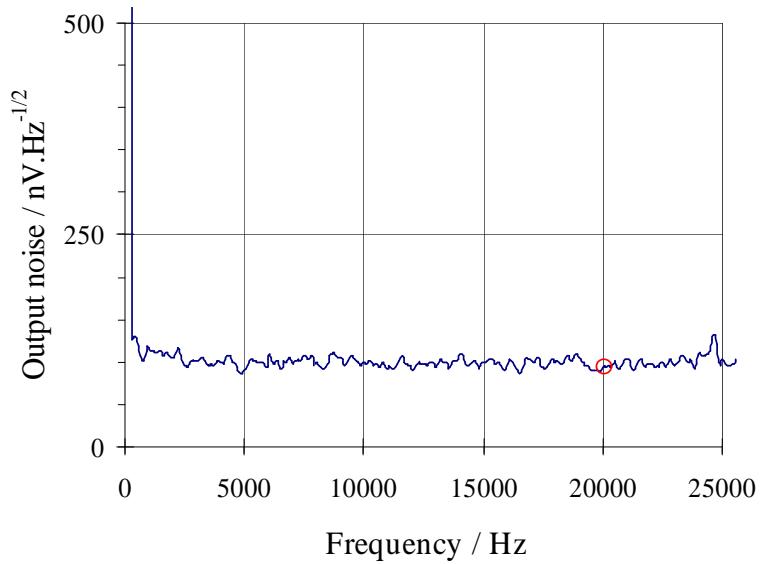


Fig. 5.1b. Typical preamplifier input shorted noise spectra at higher frequencies
Amplifier gain = x100. Noise at 20kHz = 1.0nV.Hz^{-1/2}

6. System Calibration and Test Results

The detectors are calibrated using QMC Instruments unique range of mesh filters to provide an appropriate level of signal within a known (sometimes narrow) wavelength range. A blackbody source is used to provide broad band power, which is passed through a combination of filters. This provides a measured amount of incident power on the cryostat window. A lock-in amplifier and / or signal analyser are used to measure the detector output signal.

The Ge:Ga photoconductor is calibrated using a 142cm^{-1} low-pass filter so that the response is only to a narrow band centred around the peak of its response curve.

The typical spectral responsivity of a Ge:Ga detector is shown in **Fig. A.1. in Appendix A**. This kind of detector has maximum responsivity at approximately 100cm^{-1} , above which frequency the voltage responsivity falls away in proportion to the wavelength (exactly as one expects - the detector is a photon counter).

The optical parameters that define the performance of the detector are defined below and the arrangement for the optical tests is shown in **Fig. 6.1.**

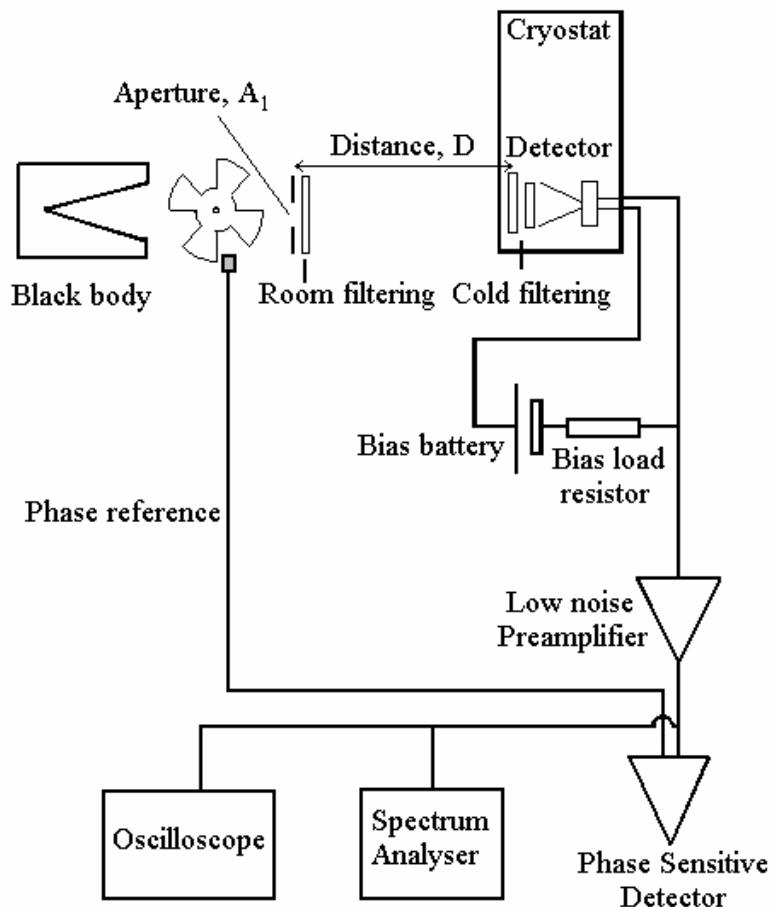


Fig. 6.1. The optical test arrangement

The system optical responsivity, R_{optical} , is defined as:

$$R_{\text{optical}} = V_{\text{out}}/P_{\text{det}}$$

where V_{out} is the voltage response at the input of the amplifier (i.e. assuming a preamplifier gain of 1) and P_{det} is the power incident on the window of the cryostat within the field of view determined by the cold optics.

The incident power, P_{det} , is calculated using

$$P_{\text{det}} = \frac{A_1 A_2}{D^2} \frac{2k\beta\Delta T}{3c^2} (\nu_2^3 - \nu_1^3)$$

where

- A_1 and A_2 are the aperture areas of the black body source and the receiving optics respectively
- D is the distance between these points
- $k = 1.38 \times 10^{-23} \text{ J K}^{-1}$ is Boltzmann's constant
- β is an attenuation factor, which accounts for the room temperature filter transmission losses and the square wave modulation
- $\Delta T = 500 \text{ K}$ is the temperature difference between the black body source temperature, $T_s = 800 \text{ K}$, and ambient temperature, $T_b = 300 \text{ K}$
- $c = 3 \times 10^8 \text{ m s}^{-1}$ is the vacuum speed of light
- ν_2 and ν_1 define the upper and lower frequency of the filter passband

The rms noise voltage N_m , generated by the detector system is measured in a 1Hz bandwidth at spot frequencies of (for example) 1kHz using a signal analyser. The noise is then referred to the input of the preamplifier so that gain is not taken into account.

The sensitivity of the system is represented by the **System Optical Noise Equivalent Power** (NEP_{opt}). It is this crucial parameter which predicts the signal/noise ratio that will be produced when a certain known signal flux density is incident at the cryostat window within the field of view. NEP_{opt} represents the power incident that will produce a voltage response equal to the noise voltage i.e. a signal to noise ratio of 1.

The System Optical N.E.P. is defined as follows:

$$NEP = N_m/R_{\text{optical}}$$

System Cryogenic Performance

The liquid nitrogen and liquid helium hold-times of the system are measured in QMC Instruments Ltd. tests and tabulated in **Table 6.1**. The liquid helium boil-off is measured over a few days to allow the internal components and radiation shields within the cryostat to reach thermal equilibrium. When equilibrium is reached the base boil-off is measured and used to determine the liquid helium hold-time of the cryostat. The hold-time indicated below is the subsequent fill hold-time. Note that a first fill will not last for as long due to the high initial boil-off when the cryostat is cooling from liquid nitrogen temperature.

In order to achieve these figures it is important that the operating instructions laid out in this manual are followed, and that care is taken to ensure that the cryostat is completely full before the liquid helium transfer is terminated.

The system test log sheet is given in **Appendix B**. This shows exactly what steps were taken to run the system and the elapsed time between each action.

Liquid helium reservoir capacity / litres	1.7
Liquid nitrogen reservoir capacity / litres	1.7
Base helium boil-off / litres of gas per min at STP	0.24
Liquid helium subsequent fill hold-time / hours	93 ± 10
Liquid nitrogen hold-time / hours	22 ± 4

Table 6.1. System cryogenic performance of the TK1813 cryostat

Detector Test Results

Table 6.2 below gives the approximate measured values of detector resistance as a function of temperature T/K as the detector is cooled. These values should be identical in both electrical polarities and are measured with a 180kΩ room temperature bias resistor in place. The measured resistances are non-rectifying

T/K	Detector resistance
300	34Ω
77	28Ω
4.2	117.9kΩ

Table 6.2. Measured detector resistance across the SMA electrical feedthrough (approx) as a function of temperature T/K

The values tabulated in **Table 6.2** are only intended as a guide. The resistance measured is very sensitive to the actual temperature of the detector element near 4.2K (dR/dT is large). This detector is a non-linear (non-ohmic) device, hence the resistance will depend on the measuring current passed through it by the measuring instrument.

Liquid nitrogen 77K shield aperture	18mm diameter
Winston Cone field of view	f/3.5 at 15mm diameter
300K window	2mm thick planar HDPE
77K shield filter	430cm⁻¹ low-pass QMMF [†]
4.2K Filter	430cm⁻¹ low-pass QMMF [†]

Table 6.3. Optical aperture sizes and filter details

[†]Refer to **Appendix C** for the transmission profile

Bias Resistance	180kΩ
Bias voltage, V_B	6.5V
Bias current, I_B	23μA [‡]
Detector voltage, V_{Det}	2.34V
Detector operating resistance R_{Op}	102kΩ

System optical responsivity	3.41kV W^{-1}
System rms output noise at 1kHz	$85\text{nV.Hz}^{-1/2}$
System rms output noise at 25kHz	$39\text{nV.Hz}^{-1/2}$
System rms output noise at 100kHz	$17\text{nV.Hz}^{-1/2}$
System Optical NEP at 1kHz	$24.9\text{pW.Hz}^{-1/2}$
System Optical NEP at 25kHz	$11.4\text{pW.Hz}^{-1/2}$
System Optical NEP at 100kHz	$4.98\text{pW.Hz}^{-1/2}$

Table 6.4. Ge:Ga Photodetector test results

‡ Refer to **5. The ULN95 Preamplifier, Altering the detector bias** for a description of the preamplifier test points settings used to take these measurements

To reduce signal noise the cryostat should be earthed properly prior to any measurements being made. An earth strap should be connected from the cryostat top plate to a good ground.

The system output noise spectrum is given in **Fig 6.2** below. It was measured using a gain of x100 on the ULN95 preamplifier.

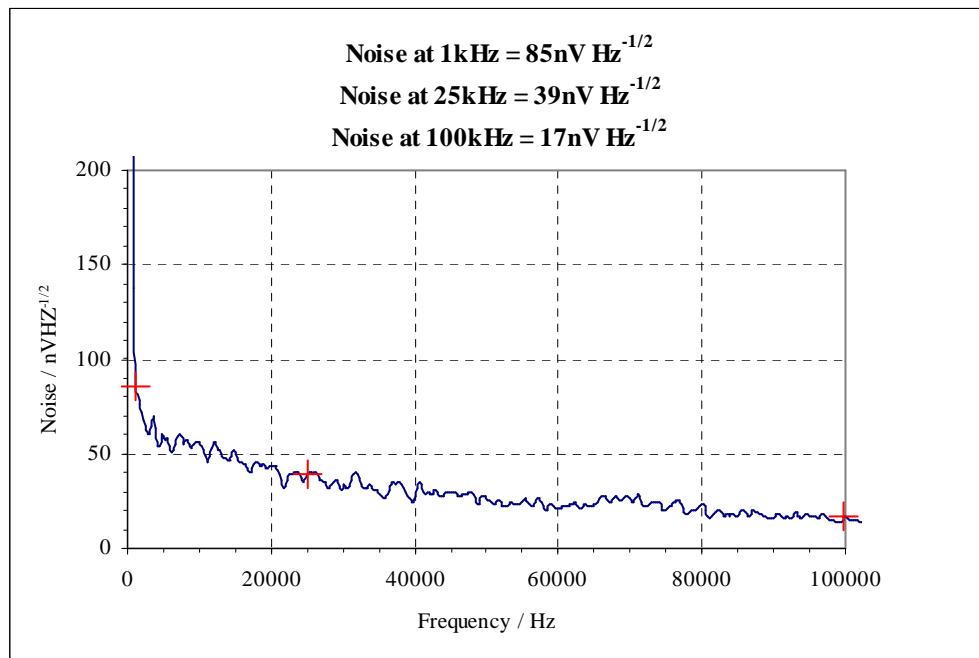


Fig. 6.2. System output noise spectrum

Appendix A. The Gallium Doped Germanium Photoconductor

The detector mounted in this system is a neutron transmuted gallium doped germanium photoconductor designed for operation at 4.2K. The active element is suspended in an integrating cavity behind the condensing optic. The incidence of photons at energies above the cut-off frequency promotes electrons into the conduction band. It is the resulting change in electrical impedance that generates a response signal.

For details of the physics of these devices the reader is referred to the following:

“Development of High Responsivity Ge:Ga Photoconductors”
N.M. Haegel et.al. Infrared Physics Vol 25, No.1 pp273-276 (1985)

The spectral responsivity of stressed and unstressed Ge:Ga photoconductor is shown in **Fig A.1** below.

Reference: Germanium Detectors for the Far-Infrared;
Erick T. Young; Steward Observatory; University of Arizona.

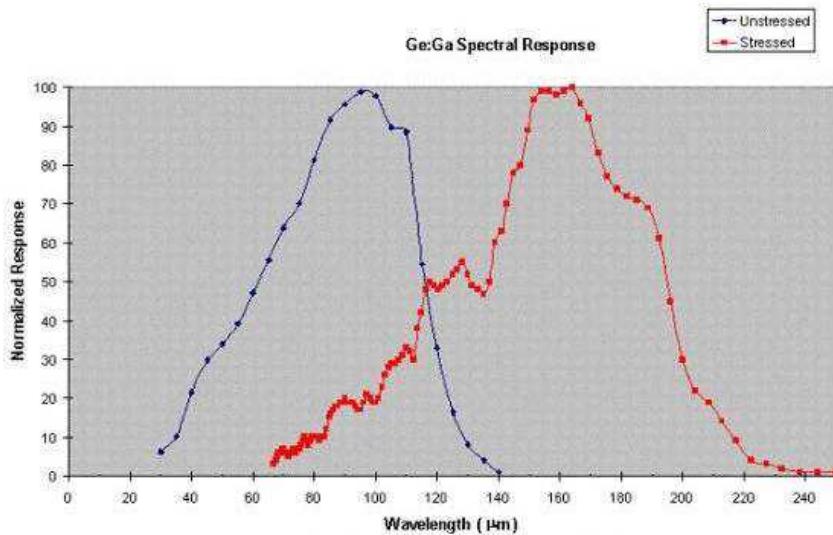


Figure 2. Spectral Response for Stressed and Unstressed Ge:Ga.

Fig. A.1. Spectral responsivity for the Ge:Ga photoconductors

Appendix C. Filter Transmission

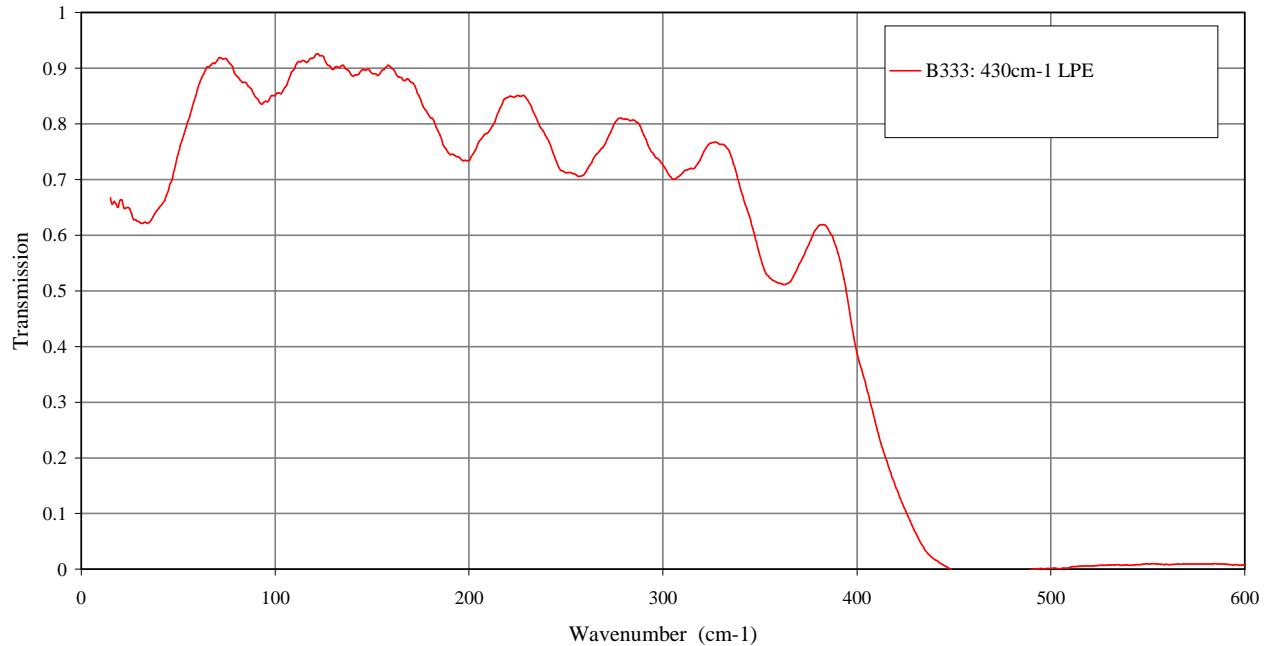


Fig C.1. Transmission spectrum for the type QMMF 430cm^{-1} low pass filter

Note: The filter transmission appears to dip below zero from about 450cm^{-1} to 500cm^{-1} . This is not real. It is caused by phasing in the Fourier Transform.

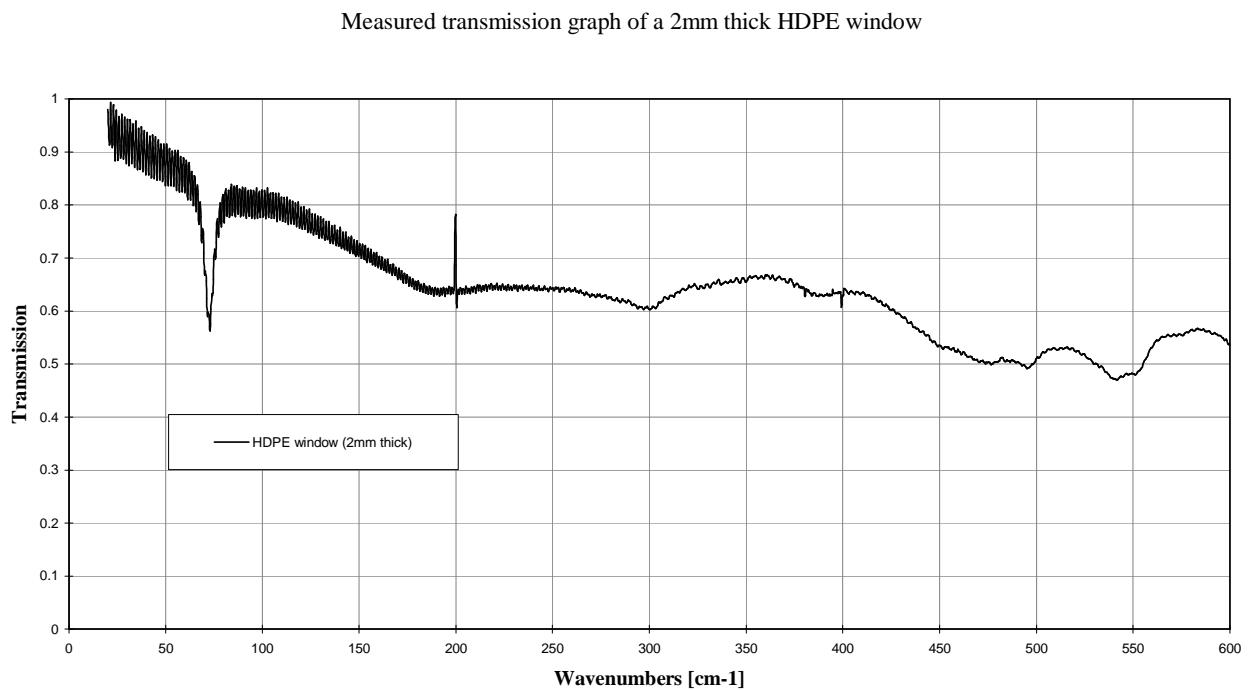


Fig. C.2. Measured transmission of a 2mm thick HDPE window from 20cm^{-1} to 600cm^{-1} .
The polyethylene characteristic absorption increase is clearly seen around 73cm^{-1}

Contract details and guarantee

This equipment is guaranteed for a period of two years from the date of delivery against failure caused by defective materials or workmanship. Defective parts will be repaired or replaced on return to the final supplier at no cost, provided that failure is not due to misuse or mishandling after delivery. QMC Instruments Limited will assume no liability for loss of life or damage to property arising from the use or misuse of its products.

Purchase Order Number

Purchase Order Date

QMCIL Reference

System Serial Number

On receipt of your shipment

Please check that your equipment has arrived safely. Please advise QMC Instruments if you suspect any damage has been incurred during transport and delivery or if any of the items are missing.

This operating manual contains instructions for operation of the preamplifier, together with QMC Instruments Ltd. test performance data, against which our guarantee is given as stated above. The user is advised to read this document carefully prior to operation of the detector system and is reminded that our guarantee will be invalidated if the equipment is damaged through misuse.

Signed..... Date.....
Ken Wood - Director, QMC Instruments Ltd

QMC Instruments technical staff will be happy to advise you if you have any questions or difficulties. The contact details are:

Ken Wood (Sales and Marketing Director)
QMC Instruments Ltd
Cardiff University
School of Physics and Astronomy
Queens Buildings
The Parade
Cardiff
CF24 3AA
UK

T. +44 (0) 29 2045 1071
F. +44 (0) 29 2045 1271
E. k.wood@terahertz.co.uk
www.terahertz.co.uk